


```

=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : GC 7890                      Location : 1 (F)
Injection Date  : 14/6/2024 8:58:28 a. m.
                                           Inj Volume : 1 µl
Acq. Method     : C:\CHEM32\1\METHODS\Calib Sec 4 Niveles Cacs.M
Last changed    : 14/6/2024 7:37:38 a. m. by SYSTEM
                 (modified after Loading)
Analysis Method : C:\CHEM32\1\METHODS\Calib Sec 4 Niveles Cacs.M
Last changed    : 14/6/2024 9:20:19 a. m. by SYSTEM
                 (modified after Loading)
Sample Info     : C.a destilería San Javier Lote F 5 Años 11 meses
  
```

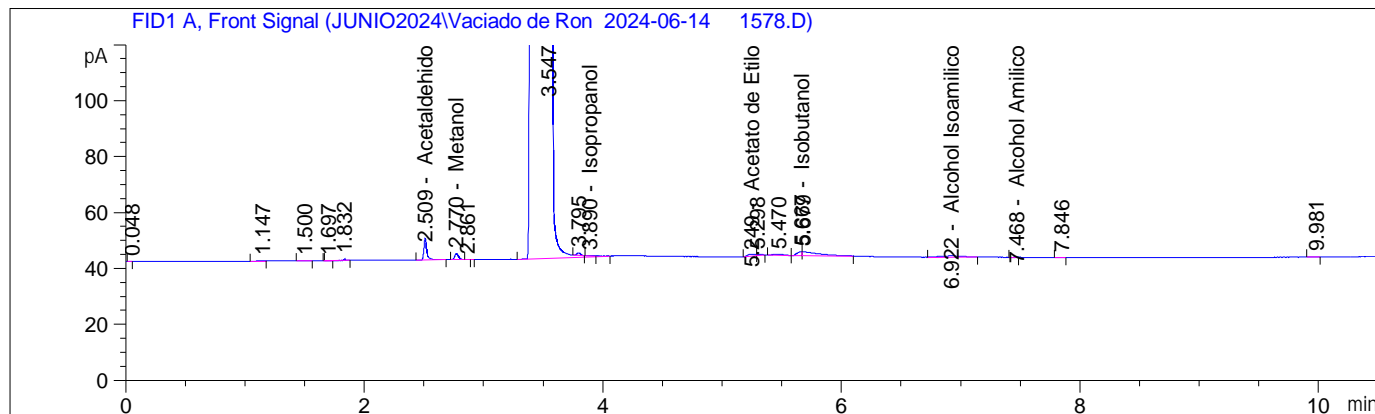

External Standard Report

```

Sorted By           : Retention Time
Calib. Data Modified : 14/6/2024 9:20:16 a. m.
Multiplier          : 1.0000
Dilution            : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: FID1 A, Front Signal

RetTime [min]	Sig	Type	Area [pA*s]	Amt/Area	Amount [ng/ul]	Grp	Name
2.509	1	BB	13.12933	1.36090	17.86773		Acetaldehido
2.770	1	BV R	4.88082	1.18336	5.77579		Metanol
3.890	1	VV T	4.70592e-1	7.93440e-1	3.73387e-1		Isopropanol
4.058	1		-	-	-		Acetato de Metilo
4.611	1		-	-	-		Propanol
5.249	1	BV	3.83914	1.54308	5.92409		Acetato de Etilo
5.667	1	BV	4.52020	5.72901e-1	2.58962		Isobutanol
6.922	1	BV R	5.62541	4.55007e-1	2.55960		Alcohol Isoamilico
7.468	1	BV	3.38479e-1	4.40967e-1	1.49258e-1		Alcohol Amilico
7.486	1		-	-	-		Furfural
8.507	1		-	-	-		Acetato de Isoamilico

Totals : 35.23947

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====
*** End of Report ***