


```

=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : GC 7890                      Location :    1 (F)
Injection Date  : 14/6/2024 9:53:33 a. m.
                                           Inj Volume : 1 µl
Acq. Method     : C:\CHEM32\1\METHODS\Calib Sec 4 Niveles Cacs.M
Last changed    : 14/6/2024 9:20:19 a. m. by SYSTEM
                 (modified after Loading)
Analysis Method : C:\CHEM32\1\METHODS\Calib Sec 4 Niveles Cacs.M
Last changed    : 14/6/2024 10:16:47 a. m. by SYSTEM
                 (modified after Loading)
Sample Info     : C.A Destilería San Javier Lote D 6 Años
  
```

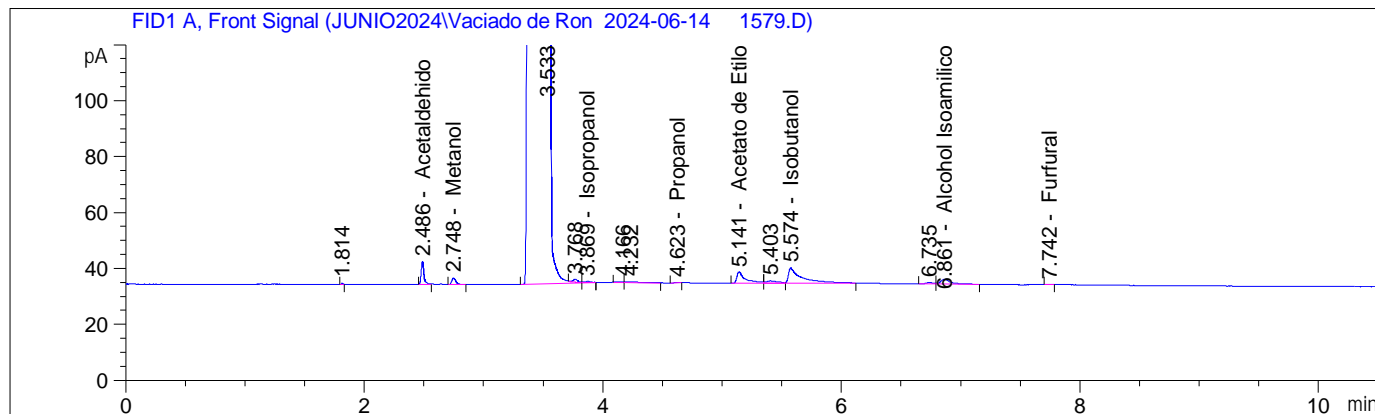

External Standard Report

```

Sorted By           :      Retention Time
Calib. Data Modified :      14/6/2024 10:16:45 a. m.
Multiplier          :      1.0000
Dilution            :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: FID1 A, Front Signal

RetTime [min]	Sig	Type	Area [pA*s]	Amt/Area	Amount [ng/ul]	Grp	Name
2.486	1	BB	12.97540	1.36090	17.65825		Acetaldehido
2.748	1	BB	5.41127	1.18336	6.40350		Metanol
3.869	1	VB E	1.17362	7.93440e-1	9.31201e-1		Isopropanol
4.058	1		-	-	-		Acetato de Metilo
4.623	1	BV	5.91497e-1	6.28111e-1	3.71526e-1		Propanol
5.141	1	BV	20.61822	1.54308	31.81548		Acetato de Etilo
5.574	1	VV R	41.80427	5.72901e-1	23.94969		Isobutanol
6.861	1	VV R	10.74060	4.55007e-1	4.88705		Alcohol Isoamilico
7.468	1		-	-	-		Alcohol Amilico
7.742	1	BB	2.57447e-1	5.98971e-1	1.54203e-1		Furfural
8.507	1		-	-	-		Acetato de Isoamilico

Totals : 86.17090

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====  
\*\*\* End of Report \*\*\*