


Sample Name: Vaciado de Ron

```

=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : GC 7890                      Location : 1 (F)
Injection Date  : 14/6/2024 10:23:42 a. m.
                                           Inj Volume : 1 µl
Method          : C:\CHEM32\1\METHODS\Calib Sec 4 Niveles Cacs.M
Last changed    : 14/6/2024 10:16:47 a. m. by SYSTEM
                 (modified after loading)
Sample Info     : C.A Destilería San Javier Lote B 7 Años 2 meses
    
```

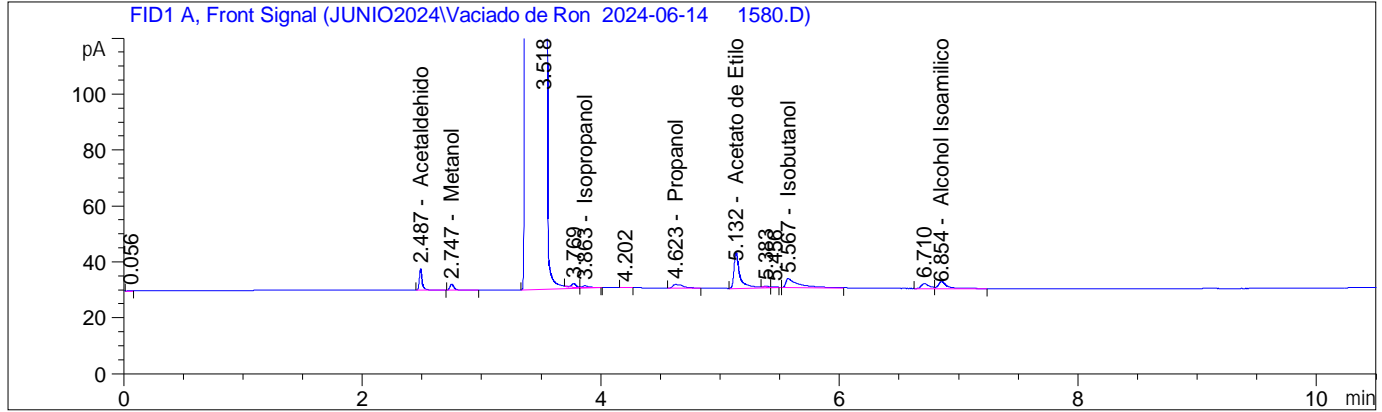

External Standard Report

```

Sorted By           : Retention Time
Calib. Data Modified : 14/6/2024 10:16:45 a. m.
Multiplier          : 1.0000
Dilution            : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: FID1 A, Front Signal

RetTime [min]	Sig	Type	Area [pA*s]	Amt/Area	Amount [ng/ul]	Grp	Name
2.487	1	BV R	13.33491	1.36090	18.14750		Acetaldehido
2.747	1	BV R	5.22150	1.18336	6.17894		Metanol
3.863	1	VB E	2.41701	7.93440e-1	1.91775		Isopropanol
4.058	1		-	-	-		Acetato de Metilo
4.623	1	BV R	7.72052	6.28111e-1	4.84934		Propanol
5.132	1	BV R	46.39497	1.54308	71.59096		Acetato de Etilo
5.567	1	BB	24.10997	5.72901e-1	13.81262		Isobutanol
6.854	1	VB	12.61386	4.55007e-1	5.73940		Alcohol Isoamilico
7.468	1		-	-	-		Alcohol Amilico
7.742	1		-	-	-		Furfural
8.507	1		-	-	-		Acetato de Isoamilico

Totals : 122.23651

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====  
\*\*\* End of Report \*\*\*